


7.3 BODY LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity (ϵ_r') | | Conductivity (σ) S/m | |
|------------------|---|----------|-------------------------------|----------|
| | required | measured | required | measured |
| 150 | 61.9 ±10 % | | 0.80 ±10 % | |
| 300 | 58.2 ±10 % | | 0.92 ±10 % | |
| 450 | 56.7 ±10 % | | 0.94 ±10 % | |
| 750 | 55.5 ±10 % | | 0.96 ±10 % | |
| 835 | 55.2 ±10 % | | 0.97 ±10 % | |
| 900 | 55.0 ±10 % | | 1.05 ±10 % | |
| 915 | 55.0 ±10 % | | 1.06 ±10 % | |
| 1450 | 54.0 ±10 % | | 1.30 ±10 % | |
| 1610 | 53.8 ±10 % | | 1.40 ±10 % | |
| 1800 | 53.3 ±10 % | | 1.52 ±10 % | |
| 1900 | 53.3 ±10 % | | 1.52 ±10 % | |
| 2000 | 53.3 ±10 % | | 1.52 ±10 % | |
| 2100 | 53.2 ±10 % | | 1.62 ±10 % | |
| 2300 | 52.9 ±10 % | | 1.81 ±10 % | |
| 2450 | 52.7 ±10 % | 53.4 | 1.95 ±10 % | 2.14 |
| 2600 | 52.5 ±10 % | | 2.16 ±10 % | |
| 3000 | 52.0 ±10 % | | 2.73 ±10 % | |
| 3300 | 51.6 ±10 % | | 3.08 ±10 % | |
| 3500 | 51.3 ±10 % | | 3.31 ±10 % | |
| 3700 | 51.0 ±10 % | | 3.55 ±10 % | |
| 3900 | 50.8 ±10 % | | 3.78 ±10 % | |
| 4200 | 50.4 ±10 % | | 4.13 ±10 % | |
| 4600 | 49.8 ±10 % | | 4.60 ±10 % | |
| 4900 | 49.4 ±10 % | | 4.95 ±10 % | |
| 5200 | 49.0 ±10 % | | 5.30 ±10 % | |
| 5300 | 48.9 ±10 % | | 5.42 ±10 % | |
| 5400 | 48.7 ±10 % | | 5.53 ±10 % | |
| 5500 | 48.6 ±10 % | | 5.65 ±10 % | |
| 5600 | 48.5 ±10 % | | 5.77 ±10 % | |
| 5800 | 48.2 ±10 % | | 6.00 ±10 % | |

7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

| | |
|---|---|
| Software | OPENSAR V5 |
| Phantom | SN 13/09 SAM68 |
| Probe | SN 41/18 EPGO333 |
| Liquid | Body Liquid Values: ϵ_p ' : 53.4 σ : 2.14 |
| Distance between dipole center and liquid | 10.0 mm |
| Area scan resolution | $dx=8mm/dy=8mm$ |
| Zoon Scan Resolution | $dx=5mm/dy=5mm/dz=5mm$ |
| Frequency | 2450 MHz |
| Input power | 20 dBm |
| Liquid Temperature | 20 +/- 1 °C |
| Lab Temperature | 20 +/- 1 °C |
| Lab Humidity | 30-70 % |

| Frequency MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|---------------|------------------|-------------------|
| | measured | measured |
| 2450 | 53.84 (5.38) | 23.26 (2.33) |

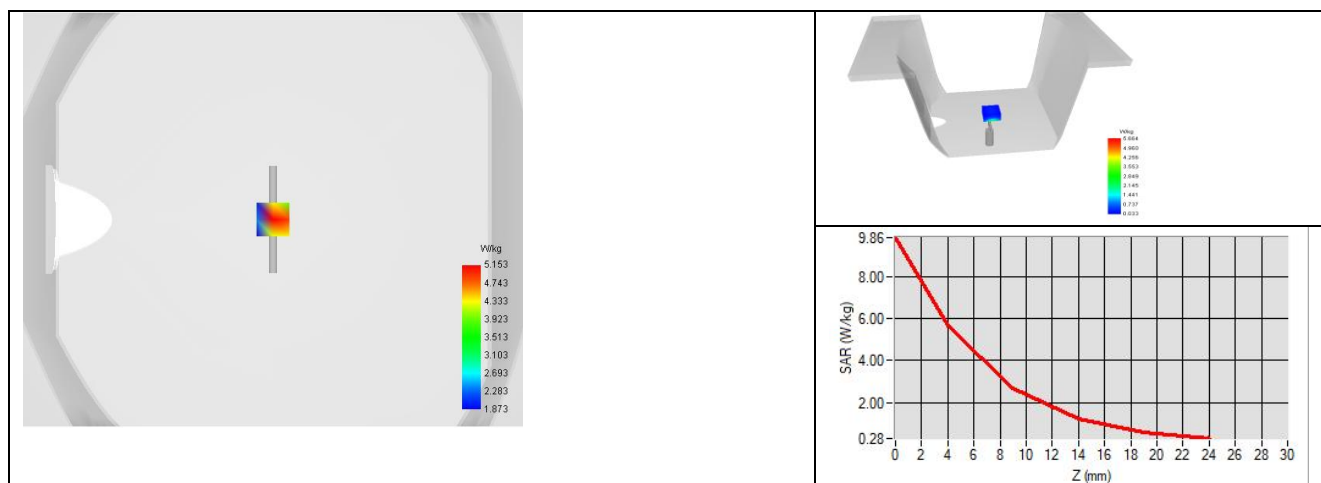



8 LIST OF EQUIPMENT

| Equipment Summary Sheet | | | | |
|------------------------------------|-------------------------|--------------------|---|---|
| Equipment Description | Manufacturer / Model | Identification No. | Current Calibration Date | Next Calibration Date |
| SAM Phantom | MVG | SN 13/09 SAM68 | Validated. No cal required. | Validated. No cal required. |
| COMOSAR Test Bench | Version 3 | NA | Validated. No cal required. | Validated. No cal required. |
| Network Analyzer | Rohde & Schwarz ZVM | 100203 | 08/2021 | 08/2024 |
| Network Analyzer | Agilent 8753ES | MY40003210 | 10/2021 | 10/2024 |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223 | 05/2021 | 05/2024 |
| Network Analyzer – Calibration kit | HP 85033D | 3423A08186 | 06/2021 | 06/2027 |
| Calipers | Mitutoyo | SN 0009732 | 10/2021 | 10/2024 |
| Reference Probe | MVG | SN 41/18 EPGO333 | 10/2021 | 10/2024 |
| Multimeter | Keithley 2000 | 1160271 | 02/2021 | 02/2024 |
| Signal Generator | Rohde & Schwarz SMB | 106589 | 04/2021 | 04/2024 |
| Amplifier | MVG | MODU-023-C-0002 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter | NI-USB 5680 | 170100013 | 06/2021 | 06/2024 |
| Power Meter | Rohde & Schwarz NRVD | 832839-056 | 11/2021 | 11/2024 |
| Directional Coupler | Krytar 158020 | 131467 | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor | Testo 184 H1 | 44225320 | 06/2021 | 06/2024 |