

Annex 4: Test setup photographs 19-1-0137401T05a-C01-A4

Number of pages: 8 Date of Report: 2021-Jun-09

Fax: +49 (0) 20 54 / 95 19-150

Testing company: CETECOM GmbH Applicant: Bosch Healthcare Solutions

Im Teelbruch 116 GmbH 45219 Essen Germany Tel. + 49 (0) 20 54 / 95 19-0

Test Object / System for quantitative measurement of fractional nitric oxide (FeNO) in human breath,
Tested Device(s): Vivatmo pro (Base Station)

FCC ID: 2AVQ9VMPBS1 IC: 25928-VMPBS1

Testing has been carried out in accordance with:

Title 47 CFR, Chapter I
FCC Regulations, Subchapter A
Subpart C: §15.247 (DTS)

RSS-247, Issue 2 (DTS) RSS-Gen., Issue 5

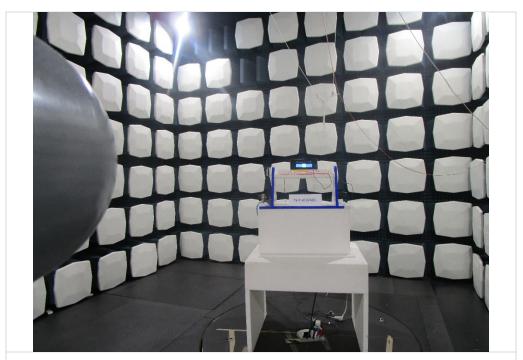


Table of Contents

1	TEST SETUP PHOTOGRAPHS	. 3
1.1	Simultaneous Emissions Test Set up photographs	6



1.1 Test setup photographs



Photograph 1: EUT Test Setup in the anechoic chamber,
Radiated interference field strength, long shot view



Photograph 2: EUT Test Setup in the anechoic chamber,


Radiated interference field strength, close-up view






Photograph 3: EUT Setup Magnetic Field Measurements in the Semi anechoic chamber,

Long shot view

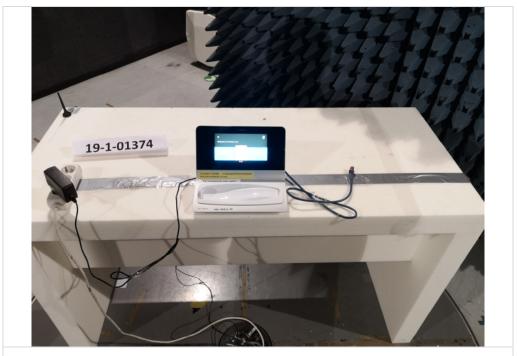

Photograph 4: EUT Setup Magnetic Field Measurements in the Semi anechoic chamber



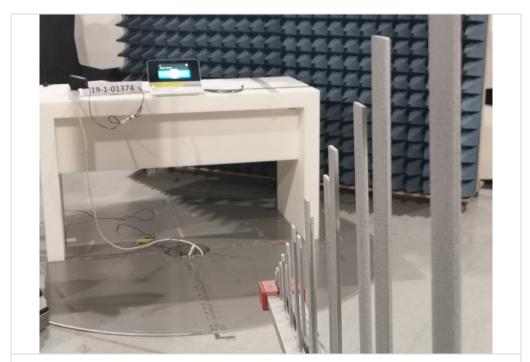

Photograph 5: EUT Test Setup in the semi-anechoic chamber,


Radiated interference field strength




Photograph 6: EUT Setup Conducted emissions on AC-Power lines



1.2 Simultaneous Emissions Test Set up photographs

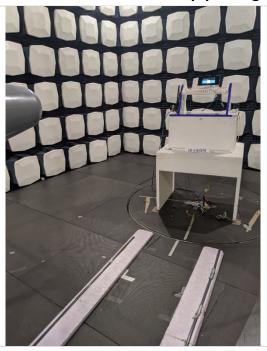

Photograph 7: EUT Test Setup in the anechoic chamber,
Radiated interference field strength, long shot view

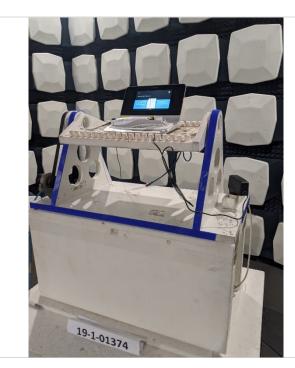

Photograph 8: EUT Test Setup in the anechoic chamber,


Radiated interference field strength, close-up view





Photograph 9: EUT Setup Magnetic Field Measurements in the Semi anechoic chamber

Long shot view

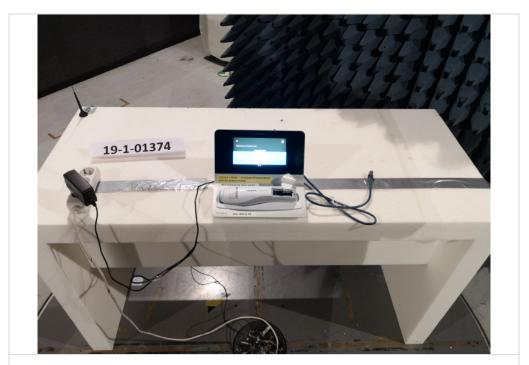

Photograph 10: EUT Setup Magnetic Field Measurements in the Semi anechoic chamber





Photograph 11: EUT Test Setup in the semi-anechoic chamber,

Radiated interference field strength



End Of Annex 4