

CS 3800

**Safety, Regulatory, and Technical
Specifications User Guide**

Notice

The Safety, Regulatory and Technical Specifications User Guide includes information on the safety instructions, regulatory information, and the technical specifications of the devices. We recommend that you thoroughly familiarize yourself with this guide to make the most effective use of your system.

© Carestream Dental LLC, 2021. The information in this document is subject to change. Neither Carestream Dental LLC nor any of its subsidiaries shall be liable for errors contained herein or for incidental damages in conjunction with the furnishing, performance, or use of this material. No part of this publication may be reproduced without the permission of Carestream Dental, LLC.

This document is originally written in English.

All trademarks and registered trademarks are the property of their respective holders.

The CS 3800 is intended for professional use only.

U.S. Federal law restricts this device to sale by or on the order of a dentist.

If any serious incident occurs in relation to the device, the user must report it to Carestream Dental and to the competent authority of its Member State in the European Union.

Manual Name: *CS 3800 Safety, Regulatory, and Technical Specifications User Guide*

Part Number: TA3977

Revision Number: 01

Print Date: 2021-05

The CS 3800 complies with Medical Device Regulation (EU) 2017/745.



Contents

Chapter 1	Indications for Use	1
Safety Information	Clinical Benefits and Performance	
	Characteristics	1
	Conventions in This Guide	2
	Warnings and Safety	
	Instructions	3
	Cleaning, Disinfecting, Sterilizing	7
	Cleaning and Disinfecting the Scanner.	7
	Cleaning the Scanner	7
	Disinfecting the Scanner.	8
	Cleaning and Sterilizing the Scanner Tips	9
	Manually Cleaning the Scanner Tips	10
	Cleaning the Scanner Tips in an Automatic Washer or Disinfector	10
	Sterilizing the Scanner Tips.	11
	Precautions Before Use	12
	Cleaning, Disinfecting, and Sterilizing.	12
	Visually Inspecting the Scanner for Damage	12
	Visually Inspecting the Scanner Tips	12
	Marking and Labeling Symbols	13
	Label Locations	14
	CS 3800 Labels	14
Chapter 2	General Regulatory Information	17
Regulatory	WiFi	20
Information	Guidance and Manufacturer's Declarations	21
	Compliance with International Regulations	24

Chapter 3	Factory25
Technical	Manufacturer25
Specifications	Model25
	CS 3800 Technical	
	Specifications25
	Length of Cables Supplied	
	with the Unit.27
	CS 3800 Environmental	
	Requirements27
	Computer System	
	Requirements28
Chapter 4	Manufacturer's Address29
Contact Information	Authorized Representatives29

1 Safety Information

Indications for Use

The CS 3800 is a digital optical scanning device used to record the topographic characteristics of teeth or dental impressions in three dimensions. The resulting topographic impressions are intended for use in the computer-aided design and manufacturing of dental restorative prosthetic devices, dental implant prosthetic devices, and orthodontic models.

Clinical Benefits and Performance Characteristics

Carestream Dental's intraoral scanners benefit a dental practice by enabling practitioners to acquire digital impressions with the quality and accuracy required for digital CAD/CAM dental applications. The actual performance of the device is dependent on the user's training and operating execution. The user is solely responsible for the accuracy, completeness, and adequacy of the acquired data.

Conventions in This Guide

The following special messages emphasize information or indicate potential risks to personnel or equipment.



WARNING: Warns you to avoid injury to yourself or others by following the safety instructions precisely.



Caution: Alerts you to a condition that might cause serious damage.



Important: Alerts you to a condition that might cause problems.



Note: Emphasizes important information.



Tip: Provides extra information and hints.

Warnings and Safety Instructions



DANGER OF ELECTRIC SHOCK

This is an electrical unit. Do NOT expose it to water spray. Such action can cause an electric shock or a malfunction of the unit.



IMPORTANT: All known residual risks, contraindications, or undesirable side effects are listed in this guide. If any serious incident occurs in relation to the device, you must report it to Carestream Dental and to the competent authority of your Member State in the European Union.



WARNINGS

CS 3800:

- You **MUST** read and understand this safety information before using the scanner.
- This scanner shall only be used inside hospitals and other professional healthcare facilities and **MUST NOT** be used near high frequency surgical equipment and the RF shielded room of an ME System for magnetic resonance imaging, where the intensity of electromagnetic disturbance is high.
- Before using the scanner, check the outer surfaces of the unit and any accessories to ensure there are no rough surfaces, sharp edges, or protrusions which may cause a safety hazard.
- You are responsible for the operation and maintenance of the scanner. You **MUST** have training to use the scanner.
- **DO NOT** place objects within the field of operation of the unit.
- When the unit is not in use, ensure that the scanner is turned **OFF**.
- **DO NOT** use the scanner in conjunction with oxygen-rich environments. This unit is not intended for use with flammable anesthetics or flammable agents.
- **DO NOT** pull or twist the cable.
- **DO NOT** drop the scanner or the accessories.

- DO NOT heat sterilize the scanner.
- DO NOT expose the scanner to water spray or submerge it in water or disinfectant.
- DO NOT expose the scanner to high vibrations.
- DO NOT expose the scanner to ultraviolet radiation directly. The scanner is not designed for ultraviolet disinfection.
- DO NOT stare at the LED emission window.
- When the tip is removed, install the rubber cover to protect the scanner lens window.
- DO NOT remove the cover of any scanner components. The scanner contains no user-serviceable parts. For any repairs, contact a qualified Carestream Dental service technician.
- DO NOT replace the cables provided with the scanner with other cables. Doing so may damage the scanner and adversely affect the safety protection and EMC performance of the scanner.
- DO NOT replace the power adapter provided with the scanner with any other power adapter. Substitutes may not provide the required protection against electric shocks and other safety hazards.
- Any other equipment not complying with IEC 60601 shall be kept at least 1.83 meters away from the patient.
- If the equipment is faulty, turn it OFF, display an “Out of Service” notice, and contact a qualified Carestream Dental service technician.
- Using components, accessories, cables, and spare parts other than those specified or provided by the manufacturer of this equipment may impair the safety protection of the scanner and may result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.
- No modification of this equipment is allowed.
- Additional multiple outlet strips or extension cords should not be connected to the system.
- The maximum temperature of the applied part may reach to 43 °C; to avoid overheating, do not use it for extended periods.
- To power off the device, push the power button for 3 seconds. To isolate the device from mains supply on all poles, unplug the adapter from the mains power outlet.
- DO NOT maintain or service this equipment while it is in use with the patient.
- Always position the unit in such a way that it is easy to disconnect the adapter from the mains power outlet.

- Connection of the PEMS (Programmable Electrical Medical System) to an IT NETWORK that includes other equipment could result in risks to patients, operators, or third parties. The responsible organization should identify, analyze, evaluate, and control these risks.

Computer:

- DO NOT place the computer and the peripheral equipment connected to it in the immediate vicinity of the patient. Leave at least 1.83 meters distance between the patient and the equipment.
- The scanner is only intended to be connected to a computer that has agency approval according to the latest edition of applicable safety and EMC standards. Connecting the scanner to other equipment may be hazardous.
- See the installation guide for your computer for information about the data processing system, computer, and screen. Leave a sufficient amount of clear space around the computer to ensure that it is properly ventilated.
- Position the screen to avoid light reflections from internal or external lighting for maximum image quality and visual comfort.

Battery:

- Do not dismantle, open, or shred secondary cells or batteries.
- Do not expose cells or batteries to heat or fire. Avoid storage in direct sunlight.
- Do not short-circuit a cell or a battery. Do not store cells or batteries haphazardly in a box or drawer where they may short-circuit each other or be short-circuited by other metal objects.
- Do not remove a cell or battery from its original packaging until required for use.
- Do not subject cells or batteries to mechanical shock.
- In the event of a cell leaking, do not allow the liquid to come in contact with the skin or eyes. If contact has been made, wash the affected area with copious amounts of water and seek medical advice.
- Do not use any charger other than that specifically provided for use with the equipment. Refer to the manufacturer's instructions or equipment manual for proper charging instructions.
- Do not use any cell or battery which is not designed for use with the equipment.
- Always purchase the battery recommended by the device manufacturer for the equipment.

- Keep cells and batteries clean and dry.
- Wipe the cell or battery terminals with a clean, dry cloth if they become dirty.
- Do not leave a battery on prolonged charge when not in use.
- After extended periods of storage, it may be necessary to charge and discharge the cells or batteries several times to obtain maximum performance.
- Retain the original product literature for future reference.
- Use only the cell or battery in the application for which it was intended.
- When possible, remove the battery from the equipment when not in use.
- Dispose of properly.

Disposal:



This equipment contains certain materials and chemical compounds incidental to the manufacture of electrical and electronic equipment, and improper “end-of-life” disposal of such equipment can result in environmental contamination. Therefore, this equipment should not be disposed of as ordinary household waste but should instead be delivered to a designated electrical and electronic waste disposal or recycling center. For further information on disposing of electrical and electronic waste, contact the cognizant authority within the local jurisdiction.

Dispose of the scanner tips according to standard operating procedures or local regulations for the disposal of contaminated medical waste. For additional scanner tips, contact your dealer.

Cleaning, Disinfecting, Sterilizing

Cleaning and Disinfecting the Scanner



WARNINGS

- Read and follow the warnings and personal protection instructions provided in the Safety Data Sheet (SDS) for the disinfectant used to process the scanner for reuse.
- You must wear gloves while cleaning and disinfecting the scanner.
- The scanner must be disinfected with an U.S. Environmental Protection Agency (EPA) registered or CE marked intermediate-level disinfectant solution with tuberculocidal activity between patients.
- DO NOT use a disinfectant containing phenolics or iodophors; doing so will damage the surface coating of the scanner.
- Never put the scanner in an autoclave device or immerse it in water or the disinfectant solution.
- Excessive fluids can damage the scanner. Do not use cotton, cloth, or tissues soaked with disinfectant to disinfect the scanner.

Cleaning the Scanner

If the scanner is visibly contaminated with blood and/or body fluids, you must clean it before disinfecting it.

To clean the scanner, follow these steps:

- 1 Dampen (**do not soak**) a lint-free cloth with lukewarm water.
- 2 Remove the blood and/or body fluids with the dampened lint-free cloth.



Caution: DO NOT touch the contact points on the battery or the scanner. Do not allow liquid to infiltrate the cover.



Disinfecting the Scanner

After each patient, the scanner must be thoroughly disinfected.

To adequately disinfect the scanner, follow the disinfectant manufacturer's instructions for the appropriate contact time.



Important: If the scanner is visibly soiled, it must be thoroughly cleaned prior to disinfecting. See ["Cleaning the Scanner."](#)

To disinfect the scanner, follow these steps:

- 1 Remove the reusable tip.
- 2 Remove all visible soil (see ["Cleaning the Scanner"](#)).
- 3 Use a commercially prepared intermediate level disinfectant wipe. Follow the manufacturer's instructions for contact time.
Approved disinfectant wipes: Mikroqid AF Jumbo Wipes, CaviWipes, Oxivir Tb Wipes, Clorox Healthcare Bleach Germicidal Wipes, PDI Sani-Cloth Bleach Germicidal Wipes.



WARNING: Using a disinfectant that has not been approved may cause damage to the scanner.

- 4 Thoroughly wipe all surfaces of the scanner. DO NOT allow liquid to enter through the gap, air outlet, or pin holes.





WARNING: Do not rinse.

- 5 Allow to air dry.
- 6 After the scanner has dried, use a clean, lint-free cloth dampened with water to remove residual disinfectant from the surface of the scanner.

Cleaning and Sterilizing the Scanner Tips

Scanner tips received from the manufacturer are NOT sterile. You must sterilize the tips before the first use.

If you limit the exposure time at 134°C to not more than 4 minutes, you can autoclave the tip up to 110 cycles.



WARNINGS

- **Wear gloves when handling a contaminated scanner tip.**
- **Read and follow the warnings and personal protection instructions provided in the manufacturer's SDS for the detergent used to clean the scanner tip prior to sterilization.**
- **Do not soak the scanner tips in disinfectant overnight.**
- **Dry the scanner tips thoroughly before mounting onto the scanner.**
- **Do not use an ultrasonic cleaning machine to clean the scanner tips.**

Manually Cleaning the Scanner Tips

To manually clean the scanner tips, follow these steps:

- 1 Rinse excess soil from the tip.
- 2 Using a soft brush, apply an enzymatic detergent solution (e.g., Metrex EmPower) to all surfaces.
- 3 Rinse under clean, running water.
- 4 Inspect the tip. If the tip is not clean, repeat the steps.
- 5 Use a lens tissue or lint-free cloth to remove any dust from the mirror in the tip.

Cleaning the Scanner Tips in an Automatic Washer or Disinfector

To clean the scanner tips in an automatic washer or disinfector, follow these steps:

- 1 Rinse excess soil from the tip.
- 2 Using a soft brush, apply an enzymatic detergent solution (e.g., Metrex EmPower) to all surfaces.
- 3 Load the tip into the washer/disinfector equipment.
- 4 Run the cycle per the equipment manufacturer's instructions.
- 5 If the machine does not have an automatic rinse cycle, rinse thoroughly to remove detergent residues by immersing in clean water.
- 6 Use a lens tissue or lint-free cloth to remove any dust from the mirror in the tip.

Sterilizing the Scanner Tips



Note: If you limit the exposure time at 134°C to not more than 4 minutes, you can autoclave the tip up to 110 cycles.

To sterilize the cleaned scanner tips, follow these steps:

- 1 Place the tip in an FDA-cleared or CE-marked sealed sterilization pouch. The pouch should be sealed air-tight. Use either a self-adhesive pouch or a heat-sealed pouch.
- 2 Place the tips in a steam autoclave for the following times:

Pre-Vacuum Autoclave		
Exposure Time at 132°C	Exposure Time at 134°C	Minimum Drying Time
Minimum 4 Minutes	Minimum 3 Minutes	20-30 Minutes

Gravity Autoclave		
Exposure Time at 132°C	Exposure Time at 134°C	Minimum Drying Time
Minimum 15 Minutes	Minimum 10 Minutes	15-30 Minutes



Important: Do NOT exceed 134°C.

Precautions Before Use

Perform the following activities on your product and accessories before use.

Cleaning, Disinfecting, and Sterilizing

To ensure maximum hygienic safety for the patient and to minimize the risk of cross-contamination, carefully perform the following maintenance activities on your scanner and accessories.

After each patient:

- Clean and disinfect the scanner. See [“Cleaning and Disinfecting the Scanner” on page 7](#).
- Clean and sterilize the scanner tip. See [“Cleaning and Sterilizing the Scanner Tips” on page 9](#).

Visually Inspecting the Scanner for Damage

Visually inspect the scanner for damage or signs of deterioration by doing the following:

- Inspect the scanner's lens window.
- Inspect around the scanner buttons and contact points.

If damage is noted, do not use the scanner and contact your representative.

Visually Inspecting the Scanner Tips

Visually inspect the scanner tips for signs of deterioration by doing the following:

- Verify that the tip is not damaged and its components are not detached.
- Verify that the tip mirror does not have any smudges or scratches on it.

If deterioration is noted, replace the tip.













WARNINGS

- **The lens window on the scanner is a delicate optical component. Mount the front protective cover to protect the lens window from damage and dirt when the scanner is not in use.**
- **The mirror in the tip is a delicate optical component. Its clean and undamaged surface is critical to scan quality.**

In the event that you see poor scan quality or an unclear video preview in the software, clean the tip mirror and the scanner's lens window using a microfiber cleaning swab, applying ethanol that is free of impurities.

Marking and Labeling Symbols

	Type BF applied part symbol classification in accordance with IEC 60601 standards.
	Class II equipment
	<p>In the European Union, this symbol indicates: DO NOT discard this product in a trash receptacle; use an appropriate recovery and recycling facility.</p> <p>Contact your local sales representative for additional information on the collection and recovery programs available for this product.</p>
	Manufacturer's address
	Manufactured date
	<p>CAUTION:</p> <p>Consult accompanying documentation.</p>
	Refer to instruction manual/booklet.
	Direct current
	Medical device
	Name of the European authorized representative and address of the registered place of business.

Label Locations

CS 3800 Labels

The following figures illustrate the label locations of the CS 3800.

Figure 1 CS 3800 Box Label



Figure 2 CS 3800 Scanner Label



Figure 3 CS 3800 Charge Station Labels

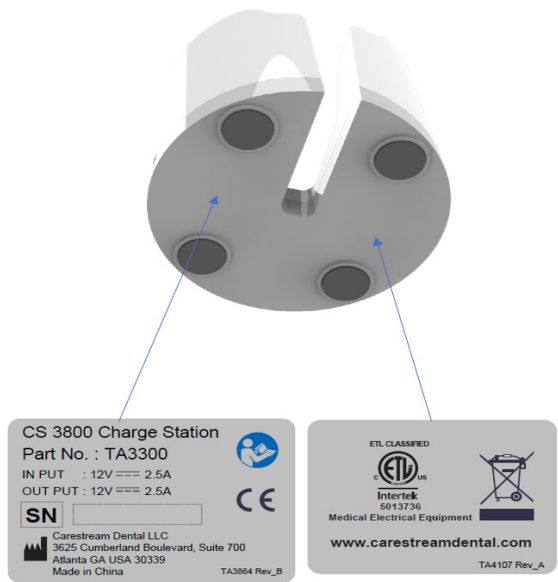


Figure 4 CS 3800 Battery Charge Station Label



Figure 5 CS 3800 Battery Label




Li-Ion : 11NR18/65

SN

3.6 V/3500 mAh

Carestream Dental LLC



2 Regulatory Information

General Regulatory Information

Compliance with European and International Standards	
EN 60601-1 / IEC 60601-1	Medical Electrical Equipment, Part 1: General Requirements for Basic Safety and Essential Performance
EN 60601-1-2 / IEC 60601-1-2	Medical Electrical Equipment, Part 1-2: General requirements for basic safety and essential performance – Collateral Standard: Electromagnetic disturbances – Requirements and tests
IEC 60601-2-18	Medical Electrical Equipment, Part 2-18: Particular requirements for the basic safety and essential performance of endoscopic equipment
EN 62471 / IEC 62471	Photobiological safety of lamps and lamp systems: Equipment classification, requirements, and User's Guide
EN ISO 17664	Processing of health care products – Information to be provided by the medical device manufacturer for the processing of medical devices
EN 60601-1-6 / IEC 60601-1-6	Medical Electrical Equipment, Part 1-6: General requirements for basic safety and essential performance - Collateral Standard: Usability
EN/IEC 62366-1	Medical Devices – Part 1: Application of usability engineering to medical devices
EN 62304 / IEC 62304	Medical device software - Software life cycle Processes

Compliance with European and International Standards	
EN ISO 10993-1	Biological evaluation of medical devices - Part 1: Evaluation and testing within a risk management process
EN ISO 14971	Medical devices - Application of risk management to medical devices
EN ISO 15223-1	Medical devices - Symbols to be used with medical device labels, labeling and information to be supplied - Part 1: General requirements
EN 1041	Information supplied by the manufacturer of medical devices
CAN/CSA-C22.2 No. 60601-1	Medical Electrical Equipment - Part 1: General requirements for basic safety and essential performance
ANSI/AAMI ES60601-1	Medical Electrical Equipment - Part 1: General requirements for basic safety and essential performance
EN 62133	Secondary cells and batteries containing alkaline or other non-acid electrolytes. Safety requirements for portable sealed secondary cells, and for batteries made from them, for use in portable applications
EN 50566	Product standard to demonstrate the compliance of wireless communication devices with the basic restrictions and exposure limit values related to human exposure to electromagnetic fields in the frequency range from 30 MHz to 6 GHz: hand-held and body mounted devices in close proximity to the human body.

Compliance with European and International Standards

EN 301 489-1	Electromagnetic compatibility (EMC) standard for radio equipment and services; Part 1: Common technical requirements; Harmonized Standard covering the essential requirements of article 3.1 (b) of Directive 2014/53/EU and the essential requirements of article 6 of Directive 2014/30/EU
EN 301 489-17	Electromagnetic Compatibility (EMC) standard for radio equipment and services; Part 17: Specific conditions for Broadband Data Transmission Systems; Harmonized Standard covering the essential requirements of article 3.1 (b) of Directive 2014/53/EU
EN 301 893	5GHz RLAN; Harmonized Standard covering the essential requirements of article 3.2 of Directive 2014/53/EU

Classification in Accordance with EN/IEC 60601-1

Type of protection against electric shock	Class II equipment
Degree of protection against electric shock	Type BF Applied Part
Mode of operation	Continuous operation
Flammable anesthetics	Not suitable for use in the presence of flammable anesthetics or a mixture of flammable anesthetics with air or oxygen or nitrous oxide.

Conformity with EN/IEC 60601-1-2

IEC 60601-1-2: 2014 EMC requirements and tests, Medical Electrical Equipment including CISPR 11:2009+A1:2010 Group 1, Class B.



Electromagnetic Compatibility Precautions

Medical electrical equipment requires special precautions regarding electromagnetic compatibility (EMC). Medical equipment must be installed and put into service according to the EMC information provided in this documentation.

Other equipment can interfere with communications with the CS 3800, even if the equipment complies with CISPR emissions requirements.

Warning: Portable and mobile RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the CS 3800, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

WiFi

The wireless version of the CS 3800 intraoral scanner operates with the 802.11 ac protocol. Only channel 42 is used for the handpiece. The central frequency is 5210MHz. The channel bandwidth is 80MHz. The radio output power is 18.5 dBm (nominal).

This equipment complies with radio frequency exposure limits set forth by the RED, the FCC, and Innovation, Science and Economic Development Canada for an uncontrolled environment.

This device complies with part 15 of the FCC Rules and contains license exempt transmitter(s)/receiver(s) that comply with Innovation, Science and Economic Development Canada's license-exempt RSS(s).

Operation is subject to the following two conditions:

- This device may not cause interference.
- This device must accept any interference, including interference that may cause undesired operation of the device.

L'émetteur/récepteur exempt de licence contenu dans le présent appareil est conforme aux CNR d'Innovation, Sciences et Développement économique Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes :

- 1) L'appareil ne doit pas produire de brouillage;
- 2) L'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.



**Caution: Changes or modifications to this unit
not expressly approved by the party responsible**

SAR Value for Handpiece:

0.46W/kg, 10g for CE;

1.594W/kg, 1g for FCC and ISED;

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

Limited by local law regulations, the version for North America does not have a region selection option.

The device is for indoor use only and operates in the 5150-5250 MHz band to reduce the potential for harmful interference to co-channel mobile satellite systems.

les dispositifs fonctionnant dans la bande de 5 150 à 5 250 MHz sont réservés uniquement pour une utilisation à l'intérieur afin de réduire les risques de brouillage préjudiciable aux systèmes de satellites mobiles utilisant les mêmes canaux.

Guidance and Manufacturer's Declarations

Guidance and Manufacturer's Declaration - Electromagnetic Immunity (IEC 60601-1-2)

The CS 3800 is intended for use in the electromagnetic environment specified below. The customer or user of the CS 3800 should assure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic Environment - Guidance
RF Emissions CISPR 11	Group 1	The CS 3800 uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment. The CS 3800 is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF Emissions CISPR 11	Class B	
Harmonic Emissions IEC 61000-3-2	Class A	
Voltage Fluctuations/ Flicker Emissions IEC 61000-3-3	Complies	

Electromagnetic Immunity for Equipment and Systems
Fully Compliant with IEC 60601-1-2: 2014

The CS 3800 is intended for use in the electromagnetic environment specified below. The customer or the user of the CS 3800 should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines	±2 kV for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line to line	±1 kV line to line	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions, and voltage variations on power supply input lines IEC 61000-4-11	0% U _T ; 0,5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270°, and 315° 0% U _T ; 1 cycle and 70% U _T ; 25/30 ^a cycles Single phase: at 0° 0% U _T ; 250/300 ^a cycles	0% U _T ; 0,5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270°, and 315° 0% U _T ; 1 cycle and 70% U _T ; 25/30 ^a cycles Single phase: at 0° 0% U _T ; 250/300 ^a cycles	Mains power quality should be that of a typical commercial or hospital environment. If the user of the CS 3800 requires continued operation during power mains interruptions, it is recommended that the CS 3800 be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

a) e.g., 10/12 means 10 periods at 50 Hz or 12 periods at 60 Hz

NOTE: U_T is the a.c. mains voltage prior to application of the test level.

Guidance and Manufacturer's Declaration - Electromagnetic Immunity (IEC 60601-1-2)

The CS 3800 is intended for use in the electromagnetic environment specified below. The customer or the user of the CS 3800 should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Electromagnetic Environment - Guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz 6 Vrms in ISM bands between 150 kHz and 80 MHz ^a	Environment of a professional healthcare facility.
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz	WARNING: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the CS 3800 including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

NOTE: Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast, and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the CS 3800 is used exceeds the applicable RF compliance level above, the CS 3800 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the CS 3800.

a The ISM (industrial, scientific and medical) bands between 150 kHz and 80 MHz are 6.765 MHz to 6.795 MHz; 13.553 MHz to 13.567 MHz; 26.957 MHz to 27.283 MHz; and 40.66 MHz to 40.70 MHz.

Guidance and Manufacturer's Declaration - Electromagnetic Immunity

For the immunity to proximity fields from RF wireless communications equipment, the CS 3800 is compliant with the test levels specified below, according to IEC60601-1-2 standard. The customer or user of the CS 3800 should assure that it is used in such an environment.

Test Frequency (MHz)	Band (MHz)	Immunity Test Levels
385	380-390	Pulse modulation 18Hz, 27V/m
450	430-470	FM, ± 5 kHz deviation, 1 kHz sine, 28V/m
710		
745	704-787	Pulse modulation 217Hz, 9V/m
780		
810		
870	800-960	Pulse modulation 18Hz, 28V/m
930		
1720		
1845	1700-1990	Pulse modulation 217Hz, 28V/m
1970		
2450	2400-2570	Pulse modulation 217Hz, 28V/m
5240		
5500	5100-5800	Pulse modulation 217Hz, 9V/m
5785		

Compliance with International Regulations

- Medical Device Regulation (EU) 2017/745
- FDA Center for Devices & Radiological Health CDRH - Title 21 CFR 872.3661 (USA)
- Medical Devices Regulations (Canada)
- Directive 2011/65/EU on the Restriction Of the use of certain Hazardous Substances in electrical and electronic equipment (ROHS), as amended by Directive (EU) 2015/863
- Radio Equipment Directive 2014/53/EU (CS 3800 Wireless only)

3 Technical Specifications

Factory

Rayco (Shanghai) Medical Products Company Limited
Building 7, No. 1510 Chuanqiao Road
China (Shanghai) Pilot Free Trade Zone
201206 Shanghai
PEOPLE'S REPUBLIC OF CHINA

Manufacturer











Carestream Dental LLC
3625 Cumberland Boulevard, Suite 700
Atlanta, GA USA 30339

Model



CS 3800 Wireless

CS 3800 Technical Specifications

Components	Technical Specifications
Sensor technology 1/2.9 inch CMOS	
Illumination	LED: Red, Blue, Green
Field of view	16 x 14 mm
	13 x 7 mm (posterior tip)
Depth of field	-2 to +16 mm

Anti-fogging technology	By airflow
Digital connection	WiFi 5GHz, 802.11ac
Handpiece dimensions	226 x 38 x 60 mm with normal tip or side tip
Components	Technical Specifications
Weight	240 g (with battery)
Handpiece	Input: 5 V  5A (with backup power cable) 4.2 V  3A (with battery)
Handpiece Charger	Input: 12 V  2.5A Output 1 (charging port): 4.2 V  3A Output 2 (port for backup power cable): 12 V  2.5A Note: When the backup power cable is attached, Output 1 is disabled, and Output 2 is enabled.
Battery Charger	Input: 12V  2.5A Output: 4.2V  3A Note: When charging a single battery, the output is 3A. When charging two batteries at the same time, the output of each slot is limited to 2.4A, to prevent the power adapter from being overloaded.
Battery	Model: 11NR18/65 3.6 V/3500 mAh
Adapter	Model LXCP30A-120: Input: 100-240V ~ 50/60Hz, 500mA Output: 12.0V  2.5A
WiFi Adapter	TP-LINK T9UH
Backup Power Cable	Length: 2m

Length of Cables Supplied with the Unit

Illustration of Part	Part Name	Length of Cable (m)
	Backup Power Cable	2.0 m
	AC Adapter	1.8 m

CS 3800 Environmental Requirements

Components	Environmental Requirements
Operating Temperature	+5 ~ 30 °C
Transportation and Storage Temperature	-10 ~ 50 °C
Operating Relative Humidity	10 – 85% RH
Transportation and Storage Relative Humidity	10 – 95% RH
Operating Atmospheric Pressure	700 – 1060 hPa
Transportation and Storage Atmospheric Pressure	600 – 1060 hPa

Computer System Requirements

If necessary, you must update your computer system configuration.

Item	Recommended	Minimum
CPU	Laptop: Intel Core i7, 9th generation	Laptop: Intel Core i7-7700HQ, Quad CPU, 2.8 GHz
	Desktop: Intel Core i7, 9th generation	Desktop: Intel Core i7-7700K, Quad CPU, 4.2 GHz
RAM	16 GB RAM	16 GB RAM
Monitor	Screen resolution: 1920 X 1080	Screen resolution: 1920 X 1080
Operating system	Windows 10 Professional, version 1809 or higher	Windows 10 Professional, version 1809 or higher
USB port	USB 3.0 for WiFi adapter	USB 3.0 for WiFi adapter
Video card	Laptop: NVIDIA GeForce RTX 2060, 6 GB memory	Laptop: NVIDIA GeForce GTX 1050 Ti or Quadro P3000 or similar
	Desktop: NVIDIA GeForce GTX 1660Ti, 6 GB memory	Desktop: NVIDIA GeForce GTX1050 Ti or similar
Video card driver	Support OpenGL 4.3 and OpenCL 1.1	Support OpenGL 4.3 and OpenCL 1.1



Note: The All-In-One computer system requirement is an exception.

The computer and its screen should be situated in or close to the operating area, in the visual field of the practitioner when using the CS 3800.



Important: It is **MANDATORY** to check that your system configuration is compatible with the computer system requirements for the CS 3800 software.



Note: Always use Microsoft Windows Update to ensure that the latest security patches are correctly installed.

4 Contact Information

Manufacturer's Address



Carestream Dental LLC
3625 Cumberland Boulevard, Suite 700
Atlanta, GA USA 30339

Authorized Representatives

Authorized Representative in the European Community



Trophy
4, Rue F. Pelloutier
Croissy-Beaubourg
77435 Marne-la-Vallée, Cedex 2
France

Authorized Representative in Brazil

Carestream Dental Brasil Eireli
Rua Romualdo Davoli, 65
1º Andar, Sala 01 - São José dos Campos
São Paulo - Brazil
CEP (Zip code): 12238-577

